

# **RTI DDS Toolkit**

**Release Notes**

**Version 4.0.0**



© 2017 - 2024 Real-Time Innovations, Inc.

All rights reserved.

Printed in U.S.A. First printing.

September 2024.

## **Trademarks**

RTI, Real-Time Innovations, Connex, Connex Drive, NDDS, the RTI logo, 1RTI and the phrase, “Your Systems. Working as one.” are registered trademarks, trademarks or service marks of Real-Time Innovations, Inc. All other trademarks belong to their respective owners.

## **Copy and Use Restrictions**

No part of this publication may be reproduced, stored in a retrieval system, or transmitted in any form (including electronic, mechanical, photocopy, and facsimile) without the prior written permission of Real-Time Innovations, Inc. The software described in this document is furnished solely under and subject to RTI's standard terms and conditions available at <https://www.rti.com/terms> and in accordance with your License Acknowledgement Certificate (LAC) and Maintenance and Support Certificate (MSC), except to the extent otherwise agreed to in writing by RTI.

## **Third-Party Software**

RTI software may contain independent, third-party software or code that are subject to third-party license terms and conditions, including open source license terms and conditions. Copies of applicable third-party licenses and notices are located at [community.rti.com/documentation](https://community.rti.com/documentation). IT IS YOUR RESPONSIBILITY TO ENSURE THAT YOUR USE OF THIRD-PARTY SOFTWARE COMPLIES WITH THE CORRESPONDING THIRD-PARTY LICENSE TERMS AND CONDITIONS.

## **Notices**

### *Deprecations and Removals*

Any deprecations or removals noted in this document serve as notice under the Real-Time Innovations, Inc. Maintenance Policy #4220 and/or any other agreements by and between RTI and customer regarding maintenance and support of RTI's software.

*Deprecated* means that the item is still supported in the release, but will be removed in a future release.

*Removed* means that the item is discontinued or no longer supported.

## **Technical Support**

Real-Time Innovations, Inc.

232 E. Java Drive

Sunnyvale, CA 94089

Phone: (408) 990-7444

Email: [support@rti.com](mailto:support@rti.com)

Website: <https://support.rti.com/>

# Contents

---

<b>Chapter 1 Supported Platforms</b> .....	<b>1</b>
<b>Chapter 2 Compatibility</b>	
2.1 DDS Toolkit Version 4.0.0 .....	2
2.2 DDS Toolkit Version 3.2.0 .....	2
2.2.1 Based on Connex 6.1.2.12 .....	2
2.2.2 DDS Toolkit is a Monolithic Library .....	2
2.2.3 ARM cRIOs not Supported .....	2
2.2.4 Security not Supported in the cRIOs .....	2
2.3 DDS Toolkit Versions 3.2.0 and Lower .....	3
2.3.1 Enums must have 32-bit Representation .....	3
2.3.2 ComplexTypes VIs must be Regenerated .....	3
2.3.3 Direct Calls through Call Library Functions No Longer Supported .....	3
2.3.4 Versions 3.1.x Incompatible with Versions Older than 2.0.0 .....	3
2.3.5 Incompatible with Connex DDS 5.1 and Lower when Using UDPv6 and Shared Memory .....	3
2.3.6 Incompatible with Connex DDS 5.0 and lower .....	4
2.3.7 Incompatibility when Regenerating Complex DataTypes Created with Version 2.0.0.104 .....	4
2.3.8 Additional Steps when Upgrading from Versions Older than 1.2.0.90 .....	4
2.3.9 Toolkit Uses String Length of 1024 .....	4
2.3.10 Improved Performance when Managing Large Data .....	5
<b>Chapter 3 What's New in 4.0.0</b>	
3.1 DDS Toolkit Based on Connex 7.3.0 .....	6
3.2 New OpenSSL version .....	6
<b>Chapter 4 Previous Releases</b>	
4.1 What's New in 3.2.0 .....	7
4.1.1 DDS Toolkit Based in Connex 6.1.2.12 .....	7
4.1.2 Toolkit Library now Includes all Dependencies .....	7

---

4.1.3	OpenSSL Replaces NI SSL .....	7
4.1.4	DDS Entities Deleted Immediately when not in Use .....	7
4.1.5	ARM cRIO Targets not Supported .....	7
4.1.6	Security Features not Supported in cRIO Systems .....	7
4.1.7	New LabVIEW Base Version Requirement .....	8
4.2	What's Fixed in 3.2.0 .....	8
4.2.1	Security may have Failed when LabVIEW 2019n SP1 or Later Installed .....	8
4.2.2	ComplexType Generator Slow to Complete when Type Definition Included Large Arrays .....	8
4.2.3	Unable to Select QoS by Topic Name .....	8
4.3	What's New in 3.1.1 .....	8
4.3.1	LabVIEW Enums are Supported Again .....	8
4.3.2	ComplexType Generator detects LabVIEW Enums and Rings with Wrong Representation .....	8
4.4	What's Fixed in 3.1.1 .....	9
4.4.1	Top-Level Member used Same Name as the Cluster with "Type" Suffix .....	9
4.4.2	Change in 3.1.0 to DataTypes of Builtin Types VIs Broke Backward Compatibility .....	9
4.5	What's New in 3.1.0 .....	9
4.5.1	Support for Arrays of Clusters .....	9
4.5.2	Support for Arrays of Strings .....	9
4.5.3	Support for Non-consecutive and Negative Enum Values .....	9
4.5.4	Ability to Read Multiple Samples with a Single Call .....	9
4.5.5	Multidimensional Arrays Mapped as Arrays, Regardless of ForceArrayMapping Option .....	10
4.5.6	Improved ComplexType Generator Checks for Type-Definition Errors .....	10
4.6	What's Fixed in 3.1.0 .....	10
4.6.1	Error 5002 when Unregistering Instance with Non-keyed String .....	10
4.7	What's New in 3.0.0 .....	10
4.7.1	New Minimum Version of LabVIEW .....	10
4.7.2	Support for Encrypted Keys .....	10
4.7.3	Ability to Show RTI Connexx DDS Core Log Messages .....	11
4.7.4	Support for Blocking Reads .....	11
4.7.5	Ability to Run Complex Type Generator Programmatically .....	11
4.7.6	Compatibility with LabVIEW Applications and Source Distributables .....	11
4.7.7	Sample Info Includes Message with Meaning of secs and nanosecs .....	11
4.8	What's Fixed in 3.0.0 .....	11
4.8.1	Continuous errors if logger queue size was zero .....	11
4.8.2	Sequences sent with fewer elements than maximum size for the sequence were not read correctly .....	11

## Chapter 5 Known Issues

---

---

5.1 Monitoring Library cannot be used as DomainParticipant's Base Profile when Creating Custom Secure Profile ..	13
5.2 No Data Received if access_scope in Publisher/Subscriber Presentation QoS is TOPIC_PRESENTATION .....	13
5.3 Warning when Closing LabVIEW after Generating VIs with ComplexType Generator or DDS Generate Custom Types VI .....	13
5.4 Built-in VIs for Reading and Writing Strings use a Fixed Size of 1024 .....	14
<b>Chapter 6 Additional Documentation .....</b>	<b>15</b>

# Chapter 1 Supported Platforms

*RTI® DDS Toolkit* is supported on these platforms:

- Windows® Systems:
  - Windows 10 (32-bit and 64-bit)
  - Windows 11 (64-bit)
  - Windows Server 2012 R2 (64-bit)
  - Windows Server 2016 R2 (32-bit and 64-bit)
- Real-Time Targets:
  - NI™ Linux® 3 on 64-bit Intel CPU (tested on cRIO-9031 target)

You will also need:

- National Instruments® LabVIEW® 2020 or later (32-bit and 64-bit)
- JKI VI Package Manager 2020 or later

# Chapter 2 Compatibility

## 2.1 DDS Toolkit Version 4.0.0

The *RTI DDS Toolkit* 4.0.0 is based on *Connex* 7.3.0.

## 2.2 DDS Toolkit Version 3.2.0

### 2.2.1 Based on Connex 6.1.2.12

*DDS Toolkit* 3.2.0 is based on *Connex* 6.1.2.12.

### 2.2.2 DDS Toolkit is a Monolithic Library

The *DDS Toolkit* library is now a monolithic library (called `rtilvdds.dll|so`) that encapsulates the previous dependencies. It also includes its own embedded OpenSSL® 1.1.1t library.

Because the monitoring and security libraries are now embedded, the methods for enabling Monitoring and Security through QoS have changed. These libraries are now enabled like static libraries. See the [Adapting a VI to Use RTI Monitoring Library and Enabling Security](#) sections of the [Getting Started Guide](#) for detailed information about these new processes.

### 2.2.3 ARM cRIOs not Supported

Version 3.2.0 does not support the ARM-based cRIO targets.

### 2.2.4 Security not Supported in the cRIOs

Version 3.2.0 does not support security in cRIO targets.



## 2.3 DDS Toolkit Versions 3.2.0 and Lower

### 2.3.1 Enums must have 32-bit Representation

Version 3.1.1 supports non-consecutive and negative values in Enums. The way an Enum is represented in a Type Definition has also changed. Now it can be represented as a “Ring” (which allows DDS Toolkit to use non-consecutive and negative values) or an “Enum” control. Rings must have an I32 representation and Enums must have a U32 representation.

### 2.3.2 ComplexTypes VIs must be Regenerated

When updating *DDS Toolkit* to version 3.1.1, the specific *ComplexTypes* VIs must be regenerated with the *RTI DDS ComplexType Generator*. These generated VIs will be compatible with the current code. Therefore, after replacing the existing custom type VIs with the generated ones, the code will work with version 3.1.1.

### 2.3.3 Direct Calls through Call Library Functions No Longer Supported

Versions of *DDS Toolkit* before 3.1.0 supported direct calls to the library by using Call Library Functions (CLFs) for compatibility with versions older than 2.0.0. This has been deprecated in 3.1.0. Direct calls using CLFs will not work anymore, even if the version is 2.0.0 or higher.

### 2.3.4 Versions 3.1.x Incompatible with Versions Older than 2.0.0

*DDS Toolkit* 3.1.0 and 3.1.1 are not compatible with versions before 2.0.0. This is due to a change described below.

Versions 3.1.0 and higher require all Custom Types to be generated using the *RTI DDS ComplexType Generator* wizard. Versions before 2.0.0 did not have this wizard, so to provide compatibility with pre-2.0.0 versions, version 3.0.0 allowed you to make direct calls to *DDS Toolkit* functions by using Call Library Functions (CLFs). However, starting with version 3.1.0, using CLFs is no longer supported. Therefore versions 3.1.0 and 3.1.1 are not compatible with versions before 2.0.0.

### 2.3.5 Incompatible with Connex DDS 5.1 and Lower when Using UDPv6 and Shared Memory

*RTI Connex*® 5.1.0 and earlier releases used a UDPv6 locator kind that was not compliant with the value in the RTPS specification. The value used in *Connex* 5.1.0 was 5 while the RTPS specification specifies a value of 2. Because of this issue, *Connex* could not interoperate with other DDS vendors over UDPv6.

This problem is resolved starting with *Connex* 5.2.0. Note, however, that out-the-box backward compatibility with *Connex* 5.1.0 and lower, when using both the UDPv6 and SHMEM transports, is broken.

For details on how to resolve this issue, see the [Connex DDS Core Libraries Release Notes for 5.2.0](#).

### 2.3.6 Incompatible with Connex DDS 5.0 and lower


In *Connex* 5.1.0, the default **message\_size\_max** for the UDPv4, UDPv6, TCP, Secure WAN, and shared-memory transports changed to provide better out-of-the-box performance.

*DDS Toolkit* 1.1.0 and higher also uses the new default value for **message\_size\_max** and therefore are not out-of-the-box compatible with applications running older versions of *Connex* (5.0 or lower) or *RTI Data Distribution Service*.

For details on how to resolve this issue, see the Transport Compatibility section of the [Connex DDS Core Libraries Release Notes for 5.1.0](#).

### 2.3.7 Incompatibility when Regenerating Complex DataTypes Created with Version 2.0.0.104

The ‘complexType’ input of the previous *Write* subVI has been changed from the 2nd left pin to the 3rd one. This doesn’t affect the functionality if the *Write* subVI is not regenerated (because it is saved and used as it was originally generated). However if you regenerate the type, the VIs that were using it will no longer be able to use it until the wire is reconnected to the correct pin.

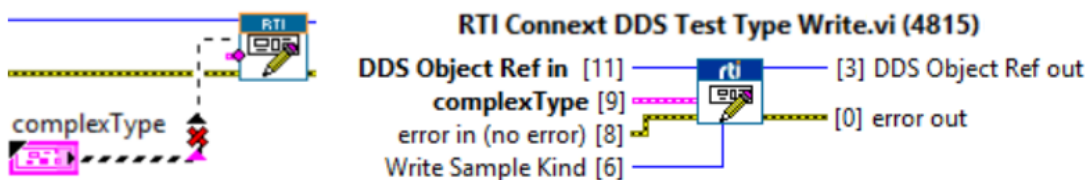

### 2.3.8 Additional Steps when Upgrading from Versions Older than 1.2.0.90

If you are upgrading from a version older than 1.2.0.90, there are important steps you must take. Briefly, changes are required because:

- The *Create Reader/Writer* subVIs have been deprecated. We strongly recommend that you upgrade the VIs to use the *Simple Create Reader/Writer* or *Advanced Create Reader/Writer*.
- The *RTI DDS Toolkit* library name changed from **lvdds.1.0.dll** to **rtilvdds.dll**.

See the *Getting Started Guide* for details on upgrading.

### 2.3.9 Toolkit Uses String Length of 1024

*DDS Toolkit* uses a default string length is 1024 characters. This may create incompatibilities with other DDS data types in your system that use string lengths  $\neq$  1024. See Section 6.2 in the *Getting Started Guide* to learn how to change the string length.

## 2.3.10 Improved Performance when Managing Large Data

We have improved the performance when managing large data by setting the following properties (note: they cannot be changed from the QoS XML file):

Dynamic data:

- **serialization.trim\_to\_size** = DDS\_BOOLEAN\_TRUE
- **serialization.max\_size\_serialized** = DDS\_LENGTH\_UNLIMITED
- **serialization.min\_size\_serialized** = TypeCode's minimum serialized size

Data Writer:

- **dds.data\_writer.history.memory\_manager.fast\_pool.pool\_buffer\_max\_size** = 1024

Data Reader:

- **dds.data\_reader.history.memory\_manager.fast\_pool.pool\_buffer\_max\_size** = 1024

# Chapter 3 What's New in 4.0.0

## 3.1 DDS Toolkit Based on Connex 7.3.0

*DDS Toolkit* 4.0.0 (specifically, this release is 4.0.0.114) is based on *Connex* 7.3.0. For information about what's new in *Connex* 7.3.0, see the [Connex 7.3.0 What's New](#) or the RTI Community Portal for 7.3.0 (<https://community.rti.com/documentation/rti-connex-730>).

## 3.2 New OpenSSL version

*DDS Toolkit* now uses OpenSSL 3.0.12.

# Chapter 4 Previous Releases

## 4.1 What's New in 3.2.0

### 4.1.1 DDS Toolkit Based in Connex 6.1.2.12

*DDS Toolkit* 3.2.0 is based in *Connex* 6.1.2.12. For information about what's new in *Connex DDS* 6.1.2, see the [Connex DDS 6.1.2 Release Notes](#).

### 4.1.2 Toolkit Library now Includes all Dependencies

*DDS Toolkit* is now built as a monolithic library that contains all the *RTI Connex* dependencies (niddscore, niddsc, rtimonitoring, niddssecurity, and rtidle libraries) and OpenSSL. For more information, see the Upgrading section of the [Getting Started Guide](#).

### 4.1.3 OpenSSL Replaces NI SSL

*DDS Toolkit* now uses OpenSSL 1.1.1t instead of NI SSL to take advantage of OpenSSL security features.

### 4.1.4 DDS Entities Deleted Immediately when not in Use

DDS entities are not preserved between different executions if all the VIs are stopped. To maintain clean executions in the development environment, all DDS entities are removed immediately when the last VI using *DDS Toolkit* stops its execution.

### 4.1.5 ARM cRIO Targets not Supported

This version does not support the ARM-based cRIO targets. Only NI Linux x64-based cRIO systems are now supported.

### 4.1.6 Security Features not Supported in cRIO Systems

*DDS Toolkit* security features are not available for use in cRIO systems.

## 4.1.7 New LabVIEW Base Version Requirement

LabVIEW 2020 is the minimum version required to use *DDS Toolkit* version 3.2.0.

## 4.2 What's Fixed in 3.2.0

### 4.2.1 Security may have Failed when LabVIEW 2019n SP1 or Later Installed

*DDS Toolkit* crashed when the security library was loaded multiple times while LabVIEW 2019 or later was installed.

[RTI Issue ID LABPLG-881]

### 4.2.2 ComplexType Generator Slow to Complete when Type Definition Included Large Arrays

*RTI DDS ComplexType Generator* took longer than expected to generate Virtual Instruments (VIs) when the Type Definition Control (ctl) file included large arrays.

[RTI Issue ID LABPLG-1017]

### 4.2.3 Unable to Select QoS by Topic Name

Choosing which QoS to use based on the topic name did not work because the topic filter was ignored. Now you can select *DataReader*, *DataWriter*, and *Topic* QoS profiles based on the evaluation of a filter expression.

[RTI Issue ID LABPLG-993]

## 4.3 What's New in 3.1.1

### 4.3.1 LabVIEW Enums are Supported Again

In version 3.1.0, LabVIEW Enums support for representing DDS Enums was removed. It was necessary to use Rings instead. In version 3.1.1, both LabVIEW Rings *and* Enums are supported. LabVIEW Enums must have a U32 representation and Rings must have an I32 representation.

### 4.3.2 ComplexType Generator detects LabVIEW Enums and Rings with Wrong Representation

While generating code, the *RTI ComplexType Generator* will now detect LabVIEW Enums with a representation other than U32, and Rings with a representation other than I32. If either are found, it will display a message with the name of the conflictive member.

## 4.4 What's Fixed in 3.1.1

### 4.4.1 Top-Level Member used Same Name as the Cluster with "Type" Suffix

In 3.1.0, the top-level cluster name was used as the top-level member name in the TypeCode. This broke backward compatibility. This problem has been resolved. In 3.1.1, the top-level member name is the TypeName. This is the same behavior as in previous versions (before 3.1.0).

[RTI Issue ID LABPLG-889]

### 4.4.2 Change in 3.1.0 to DataTypes of Builtin Types VIs Broke Backward Compatibility

In 3.1.0, builtin types VIs had different DataTypes than in previous versions. That made them incompatible with older versions. This problem has been resolved. In 3.1.1, builtin types VIs have the same DataTypes as they did before 3.1.0.

[RTI Issue ID LABPLG-936]

## 4.5 What's New in 3.1.0

### 4.5.1 Support for Arrays of Clusters

Arrays of clusters are now supported. They work the same way as regular arrays. All arrays must be initialized, including those in nested members or inside other arrays. See *Setting up Arrays*, Section 6.10 in the *RTI DDS Toolkit Getting Started Guide*, which shows how to initialize arrays.

### 4.5.2 Support for Arrays of Strings

Arrays of strings are now supported. The first string in the array specifies the length of all strings in the array (the same way as regular strings). All arrays must be initialized. See *Setting up Arrays of Strings*, Section 6.10.2 in the *RTI DDS Toolkit Getting Started Guide*, which shows how to initialize arrays of strings.

### 4.5.3 Support for Non-consecutive and Negative Enum Values

Non-consecutive values and negative values in enums are now supported. This requires you to use Rings instead of Enums in your LabVIEW control. LabVIEW Rings will be translated to DDS Enums. LabVIEW Enums are no longer supported.

### 4.5.4 Ability to Read Multiple Samples with a Single Call

The *RTI DDS ComplexType Generator* wizard generates a VI named **<Type Name> Read Array.vi**, which reads multiple samples. Its output is an array that contains the received samples. This VI

includes a “Max Samples” input, which controls the maximum number of samples that can be read at a time (use -1 to read all available samples).

### 4.5.5 Multidimensional Arrays Mapped as Arrays, Regardless of ForceArrayMapping Option

If the option **ForceArrayMapping** from the Advanced Configuration Reader/Writer was false and the Type Definitions contained multidimensional arrays, creating a Reader/Writer failed because sequences cannot be multidimensional. In version 3.1.0, multidimensional arrays are always mapped as arrays.

### 4.5.6 Improved ComplexType Generator Checks for Type-Definition Errors

To avoid erroneous VIs, the *RTI DDS ComplexType Generator* wizard now checks for issues in the Type Definition. This includes checking for unlabeled members, members in the same cluster with the same name, and LabVIEW Enums. This ensures that only VIs with supported types are generated. If any of these problems are found, the wizard reports an error message, showing the problem member and cause.

## 4.6 What’s Fixed in 3.1.0

### 4.6.1 Error 5002 when Unregistering Instance with Non-keyed String

Disposing or unregistering instances for data types that included a string that was not part of the key may have caused error 5002 to be thrown. This issue has been resolved.

[RTI Issue ID LABPLG-854]

## 4.7 What’s New in 3.0.0

### 4.7.1 New Minimum Version of LabVIEW

The minimum version of LabVIEW supported is now 2016 (instead of 2015).

### 4.7.2 Support for Encrypted Keys

This release adds support for encrypted private keys on Windows and CompactRIO™ systems. If a private key is encrypted, a password must be supplied. For more information, see the *Getting Started Guide*: Section 6.8.1, Managing Custom Security Profiles with the Security Panel (Windows Systems)” (despite the section name, this feature is also supported on CompactRIO systems) and Section 6.8.2, Managing Custom Security Profiles with SubVIs.



### 4.7.3 Ability to Show RTI Connex DDS Core Log Messages

This release includes an option to show internal *RTI Connex* core log messages. You can enable this feature in the Administration Panel.

### 4.7.4 Support for Blocking Reads

The *Read* VI now allows you to perform a read that can stay blocked until a timeout expires or a new sample arrives. This helps reduce CPU usage since there is no need to continuously poll for new samples.

### 4.7.5 Ability to Run Complex Type Generator Programmatically

The *ComplexType* Generator functionality now can be used programmatically. The Tools palette has a new VI called *DDS Generate Custom Type VIs*. This VI encapsulates the *Complex Type* Generator functionality with the same configuration parameters.

### 4.7.6 Compatibility with LabVIEW Applications and Source Distributables

*DDS Toolkit* DLL dependencies can now be packed into LabVIEW applications (.exe's) and source distributables.

### 4.7.7 Sample Info Includes Message with Meaning of secs and nanosecs

The 'DDS Sample Info' cluster includes a message with the meaning of *sec* and *nanosec*. This message is only explanatory, it does not affect the new or existing code at all.

## 4.8 What's Fixed in 3.0.0

### 4.8.1 Continuous errors if logger queue size was zero

Setting the internal logger queue size to 0 caused a continuous flow of error messages in the LabVIEW debugging window, such as:

```
LVDDS_Logger_log_new_message: Error when registering the message.
```

This problem has been resolved.

[RTI Issue ID LABPLG-720]

### 4.8.2 Sequences sent with fewer elements than maximum size for the sequence were not read correctly

When sending sequences with fewer elements than the maximum size for that sequence, a *DataReader* received values for *all* the elements in the sequence and the values were always default values. Now

#### 4.8.2 Sequences sent with fewer elements than maximum size for the sequence were not read correctly

---

sequences are read correctly.

[RTI Issue ID LABPLG-771]

# Chapter 5 Known Issues

## 5.1 Monitoring Library cannot be used as DomainParticipant's Base Profile when Creating Custom Secure Profile

When creating a DomainParticipant from a Custom Secure Profile, non-secure Monitoring cannot be enabled for that DomainParticipant. If this situation occurs, the toolkit will throw error 5080, which means that the DomainParticipant cannot be created.

[RTI Issue ID LABPLG-474]

## 5.2 No Data Received if access\_scope in Publisher/Subscriber Presentation QoS is TOPIC\_PRESENTATION

If you set the **access\_scope** in the Presentation QoS of the Publisher/Subscriber as seen below, Readers won't be able to read data:

```
<subscriber_qos>
  <presentation>
    <access_scope>TOPIC_PRESENTATION_QOS</access_scope>
    <ordered_access>true</ordered_access>
  </presentation>
</subscriber_qos>
```

[RTI Issue ID LABPLG-567]

## 5.3 Warning when Closing LabVIEW after Generating VIs with ComplexType Generator or DDS Generate Custom Types VI

In some situations, you may see a warning when closing LabVIEW after generating VIs. We recommend closing LabVIEW after generating VIs.

[RTI Issue ID LABPLG-878]

## 5.4 Built-in VIs for Reading and Writing Strings use a Fixed Size of 1024

In version 3.1.0 and higher, **SimpleCreateType\_WriterString.vi** and **SimpleCreateType\_ReaderString.vi** create a string Data Type with a fixed length of 1024. It cannot be changed by writing the desired size, as can be done in previous versions.

[RTI Issue ID LABPLG-882]

## Chapter 6 Additional Documentation

*RTI DDS Toolkit* uses *RTI Connext* for communication. For details on *RTI Connext* and the Quality of Service (QoS) settings, visit <http://community.rti.com/documentation>.